
## **Installation Note**

**Agilent Technologies 8960 Wireless Communication Test Set** 

**BBG Upgrade 1** 

Kit Part Number: E5515CU-511

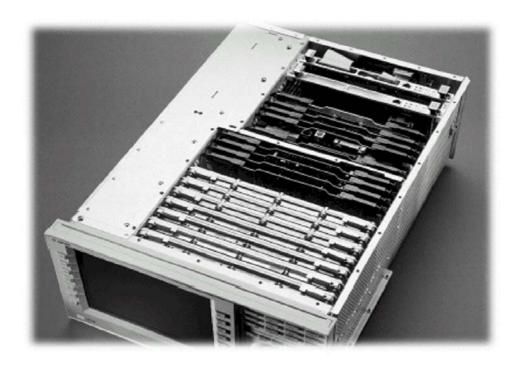

#### Notice:

The information contained in this document is subject to change without notice.

Agilent Technologies makes no warranty of any kind with regard to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.





E5515-90362

# Agilent Technologies 8960 Wireless Communication Test Set BBG Upgrade 1

Kit Part Number: E5515CU-511

 Product Affected:
 E5515C

 Replaces Board:
 E5515-60120

Applications Supported: . . . . . All current applications

To Be Performed By: . . . . . . . . (X) Agilent Technologies Service Center

(X) Personnel Qualified by Agilent Technologies

**Estimated Installation Time:** 0.5 hours **Estimated Verification Time:** 0.5 hours

#### Introduction

This kit provides the instructions for installing E5515CU-Opt 511 BBG into the E5515C Wireless Test Set. This module will enable E5515 EGPRS capabilities and associated features.

**NOTE**: This upgrade kit requires the installation of the most current revisions of application software that is compatible with this HW. Failure to install compatible applications may result in boot-up failures.

**NOTE**: It is assumed that the E5515 is fully operational prior to a HW upgrade. Installing HW upgrades in a non-operational instrument may complicate a successful installation and verification process.

If this kit is one of several HW options being installed, the following installation sequence is recommended. The actual installation will depend on the specific HW option kit(s) being installed:

- 1) Bottom section RF modules (RFIO, Attenuators)
- 2) Top section RF modules (Vector, Synth Doubler, BBG)
- 3) Digital modules (ADC, DSP, RTI, LSS, Protocol)
- 4) Rear section modules (HDD, Host Processor, Rear Panel)

#### Installation Kit Parts List

Item	Qty	Description			
1	2	TDMA Baseband Generator			
2	1	Installation Note (this document)			

#### **Tools Required**

T-20 driver

© Copyright 2008, Agilent Technologies Inc.

## Safety Considerations

**WARNING:** Before you disassemble the test set, turn the power switch off and unplug

the power cord. Failure to unplug the test set can result in personal injury.

CAUTION: Electrostatic discharge (ESD) can damage or destroy electronic

components. All work on electronic assembles should be performed at a

static-safe workstation.

## Install Compatible Versions of Existing Applications:

Upgrade all existing compatible applications to the latest revision.

- HW compatibility info is available at: <a href="https://www.agilent.com/find/e5515releasenotes">www.agilent.com/find/e5515releasenotes</a>
- Test Application downloads are available at: www.agilent.com/find/8960TA
- Lab Application downloads are available at: <a href="https://www.agilent.com/find/8960upgrades">www.agilent.com/find/8960upgrades</a>
  - 1. Make active one of the new application versions. This will ensure the instrument will boot to a compatible application after the HW installation.
  - 2. Follow the Firmware installation instructions that come with the Applications

## Remove Non-compatible Applications:

- 1. Remove all non-compatible applications from the test set. Removing older application revisions prevents improper operation of the test set. The test set must be connected to a PC using a cross-over cable via the test set's LAN port.
  - a. Run the Agilent 8960 File Utility
  - b. Select the Direct Connection (Single test set) button.
  - c. Select the Test Application tab.
  - d. Highlight the old revision(s) of application(s) and select the Delete From test set button. All licenses should remain on the instrument. Removing an application does not remove the license for that application.

## HW Disassembly:

## Remove outer cover and top cover for the 8960:

- 1. Remove handles and rear bumpers.
- 2. Remove the screws on the real panel holding outer cover.
- 3. Slide outer cover off.
- 4. Remove the 26 screws holding the top cover on and remove the cover.

#### Remove the old board:

 Remove both Baseband Generator modules. These are inserted in module slots nine and ten (counting from the front of the instrument).

© Copyright 2008, Agilent Technologies Inc. **Printed in Malaysia** 

## HW Assembly:

#### **Install Board**

1. Install the new Baseband Generator modules into the same module slots.

### Replace covers:

- 1. Replace the top cover and secure it with the 26 screws.
- 2. Slide the outer shroud (cover) on.
- 3. Replace the screws on the rear.
- 4. Attach the rear bumpers and handles.

## Verification Test after all HW Upgrades are Installed

- 1. Turn on the E5515. The unit should boot to the new Application.
- 2. Check for boot up and/or error messages. If any error message are displayed, re-check installation process for errors.
- 3. After warming up the instrument for at least 30 minutes, perform the user calibrations.

#### Calibration Procedure for Instruments with Option 003

		Calibration Int	erval = 1 year	Calibration Interval = 1 month			
Application or Format	IQ Calibrations (See Note 1)	Burst Mod Offset 1 Calibration	Thermal Power Null Adjust	Digital Average Power Calibration	Spectrum Monitor Calibration	Channel Power Calibration	Calibrate Measurements
Cdma2000/ IS-95/AMPS	Step 1 Perform IQ1and IQ2 once from one of these applications or	Step 2 Perform once from one of these applications or formats	Step 3 Perform once from one of these applications or formats	Step 4A Perform once from one of these applications or formats Step 4B Cycle Power	Step 5 Perform once from one of these applications or formats	Covered by Step 5 (See Note 2)	
1xEV-DO							
W-CDMA	formats				Step 6 Perform once from this application		Covered by Step 6 (See Note 2)
GSM/GPRS/ EGPRS					Step 7 Perform once		
AMPS/136					from one of these applications or formats		

Note 1 – Calibrate Second IQ Modulator only applies to instruments with Option 002: RF Source 2. Note 2 – You do not need to run this calibration if Spectrum Monitor calibration is run first.

#### Calibration Procedure for Instruments without Option 003

	Calibration Interval = 1 year	Calibration Interval = 1 month			
Application or Format	IQ Calibrations (See Note 1)	Spectrum Monitor Calibration			
GSM/GPRS/EGPRS	Step 1 Perform IQ1and IQ2 once from	Step 2 Perform once from one of these			
AMPS/136	one of these applications or formats	applications or formats			
Note 1 – Calibrate Second IQ Modulator only applies to instruments with Option 002:RF Source 2					

© Copyright 2008, Agilent Technologies Inc.

Printed in Malaysia Revision Date: August18, 2008

- 4. If additional verification testing is desired, tools are available from Agilent to verify the functional and parametric performance of the instrument.
  - a. Self Test software requires no external test equipment. Good for functional verification if traceable parametric measurements are not required. For more information, see <a href="http://wireless.marketing.agilent.com/docloader.asp?did=12376">http://wireless.marketing.agilent.com/docloader.asp?did=12376</a>
  - b. Test Set Verify software and system requires external test equipment. Best for traceable functional verification parametric measurements. For more information, see <a href="http://www.spk.agilent.com/~yerxa/Upgrades/index.htm">http://www.spk.agilent.com/~yerxa/Upgrades/index.htm</a>

Questions and concerns contact Agilent Technologies Support:

Phone: (800) 827-3848 (U.S. & Canada) Web: www.agilent.co